

TB-6-75
(1-8)

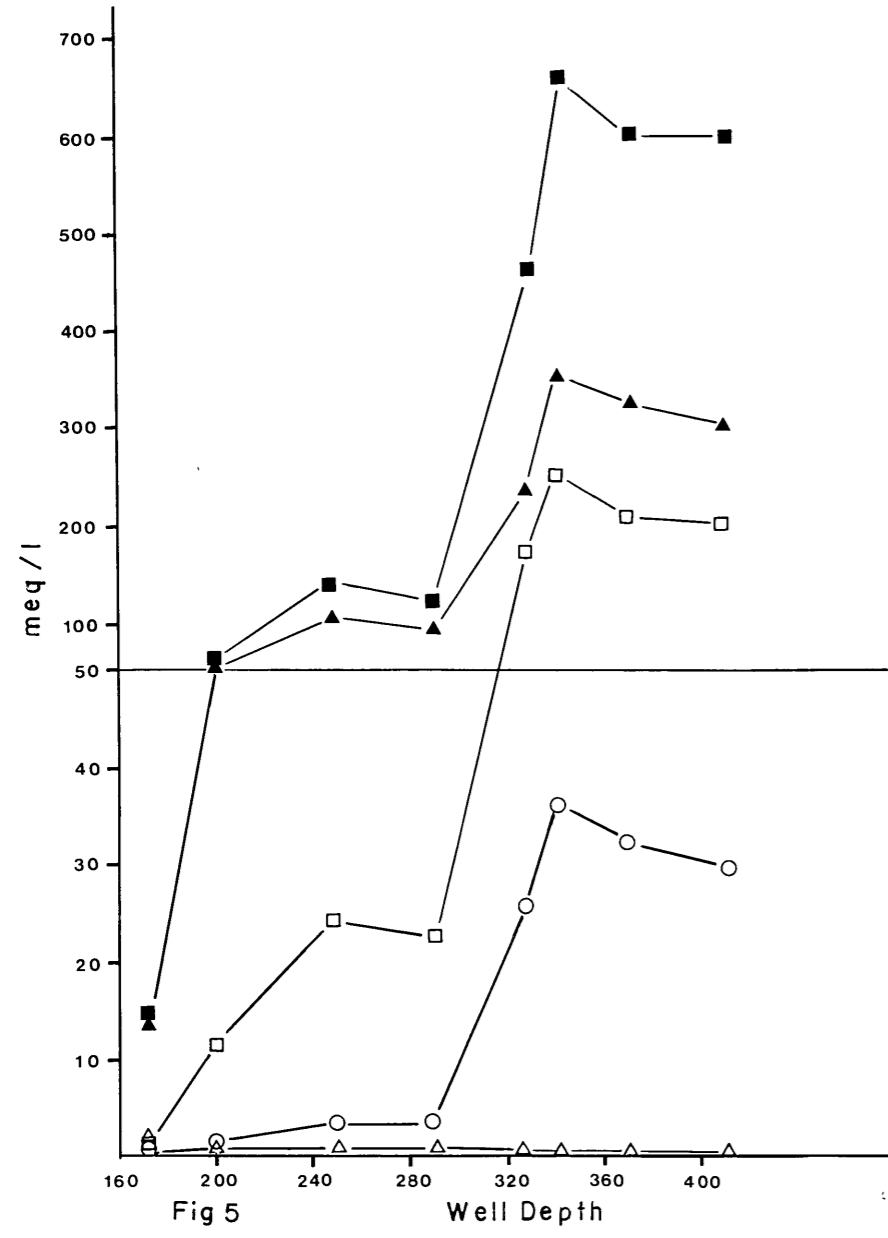


Fig 5

TB-4-75
(1-4)

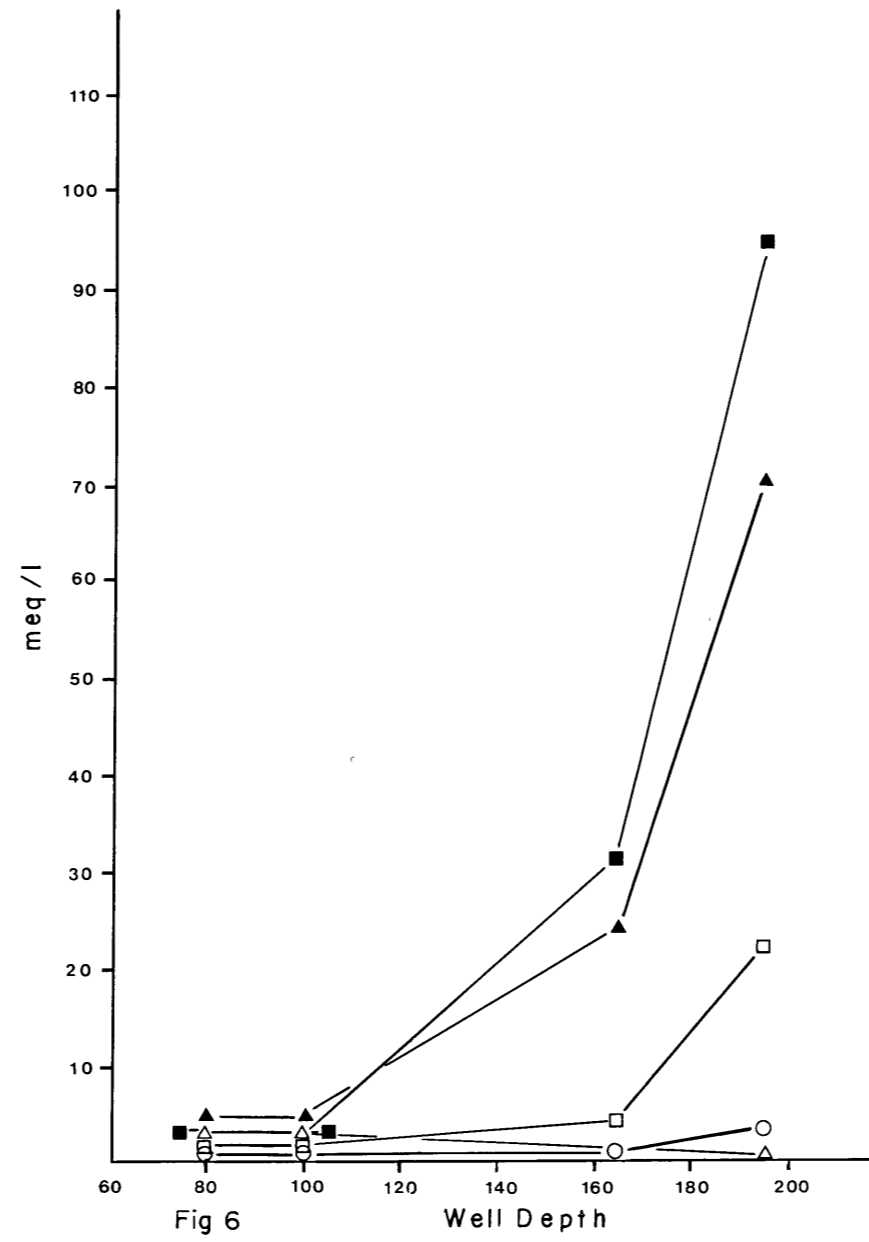


Fig 6

KEY

- ▲ Sodium
- Calcium
- Magnesium
- Chloride
- △ Alkalinity
- ⌋ Blow Test 2 hr at 200'
- (1-3) Sample 1 to 3 Table 8

TB-1-75
(1-6)

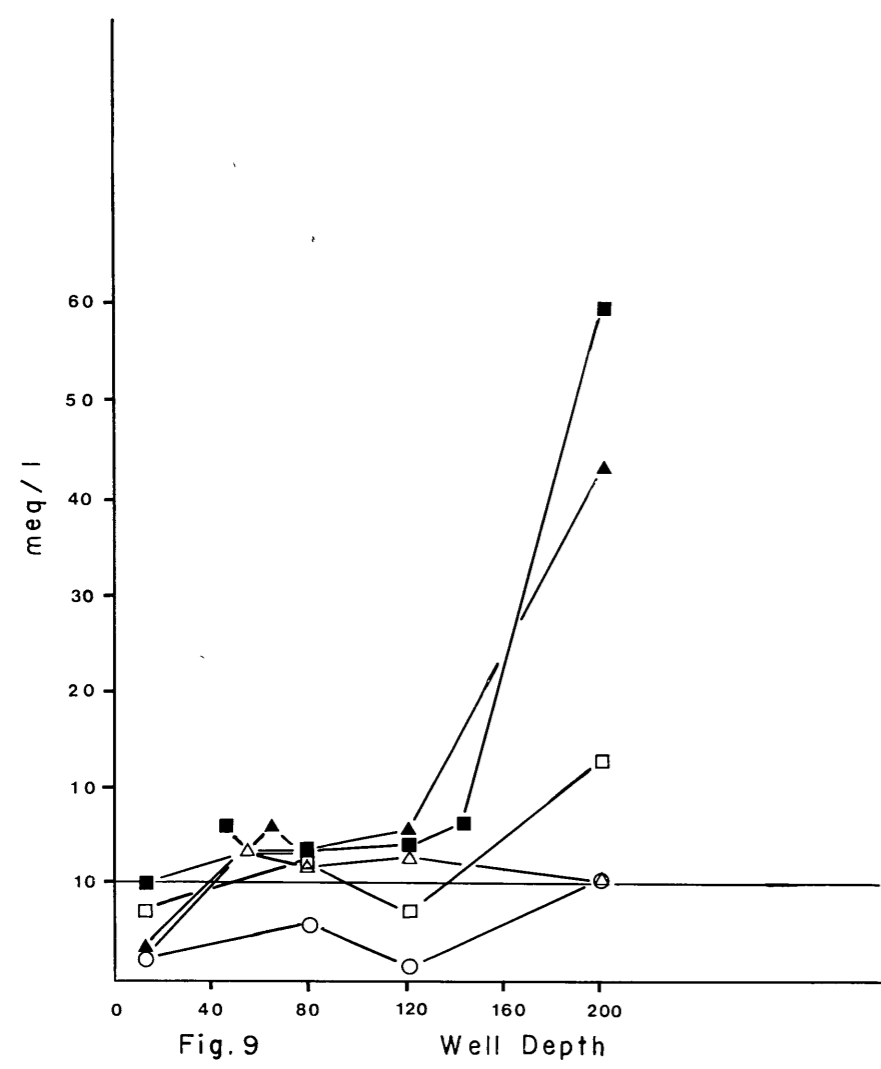


Fig. 9

TB-2-75
(1-4)

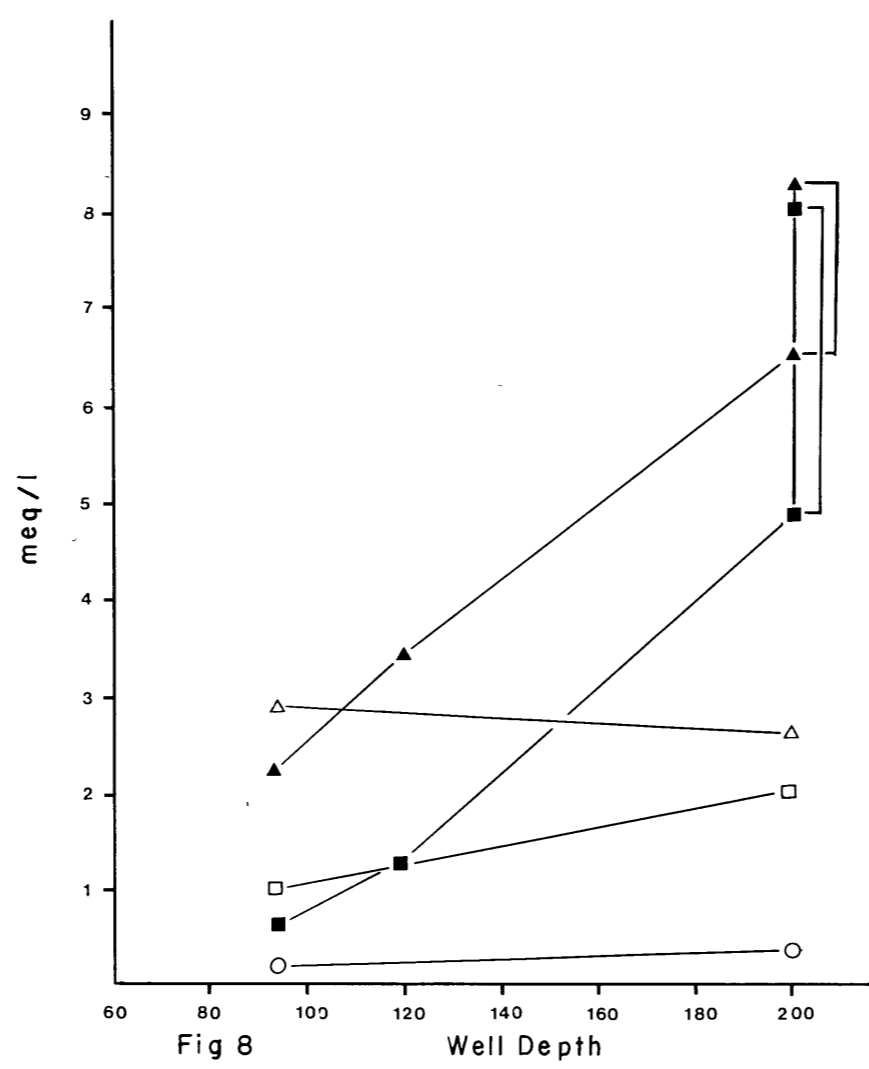


Fig 8

TB-3-75
(1-3)

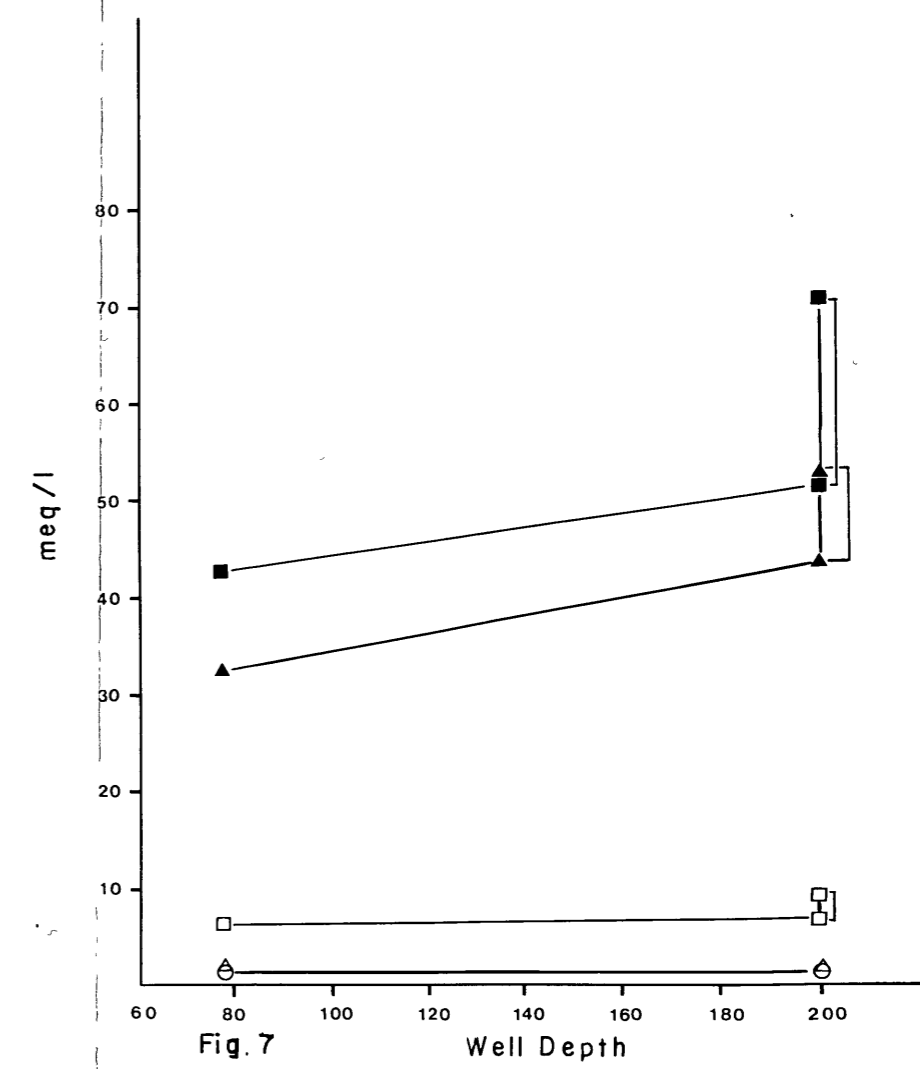


Fig. 7